

TELEVAC TELEVAC TELEVAC TELEVAC

INSTRUCTION MANUAL



MC 300 2A & 4A DUAL CHANNEL THERMOCOUPLE / CONVECTION VACUUM MEASUREMENT INSTRUMENT


TELEVAC
A DIVISION OF THE FREDERICKS COMPANY
2400 PHILMONT AVENUE,
HUNTINGDON VALLEY, PA 19006

Phone:(215) 947-2500 fax:(215) 947-7464 e-mail: sales@televac.com web site:www.televac.com
6-8000-002 REV A


PARTS LIST




1

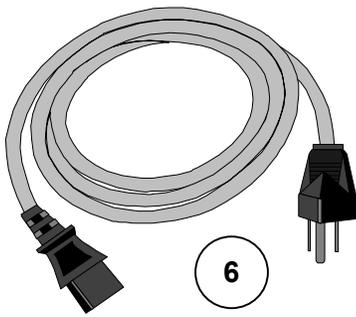

6

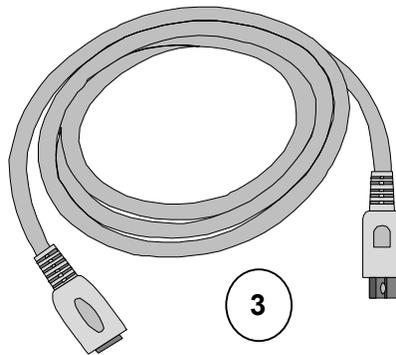


3

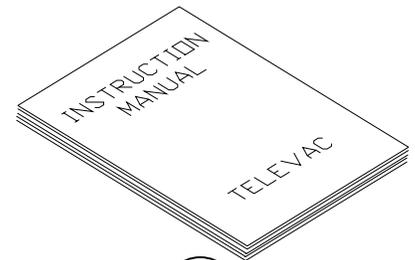

2



5

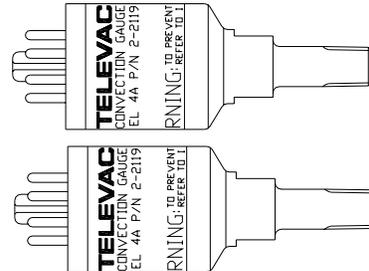

4

#	QTY	ITEM DESCRIPTION
1	1	MC300 Thermocouple, Convection, Measurement Instrument
2	1	Instruction Manual
3	3	Sensor Cables (sold separately)
4	4	Sensors (sold separately)
5	1	Mounting kit
6	1	AC Power Cable

TABLE OF CONTENTS

SECTION & TITLE

- 01. DESCRIPTION**
- 02. SAFETY INSTRUCTIONS**
- 03. PRINCIPLES OF OPERATION**
- 04. INSTALLATION & OPERATION**
- 05. ANALOG RECORDER OUTPUTS**
- 06. MAINTENANCE**
- 07. CALIBRATION**
- 08. CALIBRATION VERIFICATION**
- 09. TROUBLESHOOTING**
- 10. DIMENSION**
- 11. SPECIFICATIONS**
- 12. UNPACKING & INSPECTION**
- 13. WARRANTY INFORMATION**
- 14. ORDERING INFORMATION**

PLEASE READ THIS MANUAL THOROUGHLY BEFORE USING THIS INSTRUMENT. REPORT ANY PROBLEMS IMMEDIATELY.

Description

The TELEVAC Series MC300 vacuum-measuring instrument is a combination sensor, which incorporates various range options, as shown in the table below:

Range of Options

<u>Model</u>	<u>Range</u>	<u>Sensors</u>
MC300 2A	0 - 20,000 millitorr	2A Thermocouple
MC4A	0 – Atmosphere	4A Convection

- ✱ The 2A thermocouple gauge tube will monitor pressures between 1 millitorr (1 micron) and 20,000 microns).
- ✱ The 4A convection sensor tube will monitor pressures between 1 millitorr (1 micron) and 999 Torr. (1 atmosphere = 760 Torr @ sea level).

The vacuum measuring system consists of various gauge tubes, which sense the vacuum, an electronics unit and interconnecting signal/power cables. The customer must supply power at 115VAC 50-60 Hz. (220 Volt operation is a factory selectable option). The measured vacuum is displayed on the front panel LED displays. **(See figure 1)**

The power cable, gauge tubes, relay outputs and output voltages of 0 to 10 VDC connections are on the back panel. **(See figure 2)**



Figure 1

Figure 2



The MC300 FEATURES

- ✚ Large bright LEDs
- ✚ Built-in self-diagnostics
- ✚ Selectable Units (Torr, microns, mBar or Pascal)
- ✚ Gas compensation (Argon/Air-Nitrogen)
- ✚ Four process relays with individual assignable set points
- ✚ Analog outputs for each sensor
- ✚ Operator lockout switch

Theory of Operation:

The MC300 is a microprocessor-controlled instrument utilizing modern data acquisition techniques to achieve a high degree of accuracy at a reasonable cost.

The microprocessor in the instrument performs two basic tasks:

1. Controls the acquisition and conversion of all sensor data
2. Processes all operator interface inputs and requests

After power is applied to the instrument, the software initializes all of the circuitry associated with acquiring and displaying sensor information then performs a self-diagnostic. If there are no errors detected, the MC300's data acquisition process is started. Both input channels are read periodically and a reading for each sensor is stored. After several readings the data is averaged, then converted using the appropriate sensor, units and gas compensation settings. Set point relays and the microprocessor controlled Analog outputs are also updated at the same time. This method of averaging samples results in a smooth and accurate transition from reading to reading.

Each sensor has its own conversion algorithm. The data conversion process always occurs regardless of the instrument mode (operation set-up). However, during the set-up mode the converted data is not sent to the display but the set-point relay control and analog output operations continue to operate.

Whenever the instrument software is not processing sensor data for the displays or recorder outputs, the Set-Up, Test/Operate and Up & Down (if enabled) buttons are checked for operator interaction. The Set-Up button is used to sequence through all of the operator settable parameters. Each depression of the Set-Up button may change the function of the displays as well as the Up & Down buttons. Each time the Set-Up button is pressed, the data from the previous level is stored in non-volatile memory to ensure that the instrument's gas compensation, units and set point parameters are preserved. This information is used to restore the instrument's configuration each time power is applied.

For simplicity, the Up & Down buttons are enabled and disabled at the proper time to prevent the operator from entering an invalid value. In addition, each time an On Point is adjusted, the corresponding Off point is verified to ensure that it is higher than the new On Point. If lower, the Off Point is adjusted to be one increment higher than the new On Point. In this instance both the On and the Off Point values are updated in the non-volatile memory.

When "GAS" is selected in SETUP, a correction is applied to the instrument readings to compensate for the use of Argon as a gas instead of nitrogen/air. Both the displayed readings and the set point calibrations are compensated as well as the linear thermocouple and the linear by decade convection gauge recorder outputs at the back panel. Note, however, that the "traditional" thermocouple, "linear" convection gauge outputs and ion gauge outputs are NOT compensated.

Safety Instructions

START BY READING THESE IMPORTANT SAFETY INSTRUCTIONS AND NOTES collected here for your convenience and repeated with additional information at appropriate points in these instructions.



These safety alert symbols in this manual or on the Product rear panel mean cautions - personal safety, property damage or danger from electrical shock. Read these instructions carefully.

In these instructions the word “product” refers to the MC300 and all of its approved parts and accessories.

NOTE: *These instructions do not and cannot provide for every contingency that may arise in connection with the installation, operation, or maintenance of this product. Should you require further assistance, please contact Televac at the address on the title page of this manual.*

This product has been designed and tested to offer reasonably safe service provided in it’s installed, operated and serviced in strict accordance with these safety instructions.



Failure to comply with these instructions may result in serious personal injury, including death, or property damage.

- These safety precautions must be observed during all phases of operation, installation, and service of this product.
- Failure to comply with these precautions or with specific warnings elsewhere in this manual violates safety standards of design, manufacture, and intended use of the instrument. Televac disclaims all liability for the customer’s failure to comply with these requirements.



The service and repair information in this manual is for the use of Qualified Service Personnel. To avoid shock, do not perform any procedures in this manual or perform any Servicing on this product unless you are qualified to do so.

● ***READ Instructions:***

Read all safety and operating instructions before operating the product.

● ***RETAIN instructions:***

Retain the Safety and Operating Instructions for future reference.

● ***HEED warnings:***

Adhere to all warnings on the product and in the operating instructions.

● ***FOLLOW instructions:***

Follow all operating and maintenance instructions.

● ***ACCESSORIES:***

Do not use accessories not recommended in this manual as they may require a technician to restore the product to its normal operation.



To reduce risk of fire or electric shock, do not expose this product to rain or moisture.



Objects and Liquid Entry – Never push objects of any kind into this product through openings as they may touch dangerous voltage points or short out parts that could result in a fire or electric shock. Be careful not to spill liquid of any kind onto the products.



Do not substitute parts or modify instrument.

Because of the danger on introducing additional hazards, do not install substitute parts or perform any unauthorized modifications to the product. Return the product to Televac for service and repair to ensure that safety features are maintained. Do not use this product if it has unauthorized modifications.

Principles of Operation

2A Thermocouple Sensor



Figure 3
2A Thermocouple Sensor Tube

The 2A thermocouple sensor tube consists of a metal shell containing fine wire filaments of dissimilar metals, which form a thermocouple. The thermocouple sensor measures absolute pressures by determining the temperature of a thermocouple junction as the surrounding pressure changes. The response of the sensor depends on the gas pressure and type.

The range of these sensors is from 1 millitorr to 20,000 millitorr (10⁻³ Torr to 20 Torr). The sensor housing is constructed of stainless steel or alternately nickel plated brass. Both are capable of withstanding 150 psi overpressure.

Convection Sensor

The convection sensor measures absolute pressures by determining the heat loss from a thermocouple heated to a constant temperature by a current source. A second thermocouple compensates for ambient temperature changes and extends the vacuum measurement range above 2 Torr by measuring the convection effects. The range of these sensors is 1 millitorr to 1000 Torr

The convection sensor must be mounted vertically for accurate measurements. Sensors are available in Stainless Steel or Nickel plated Brass and can withstand 150-psi overpressure.

Figure 4
4A Convection Sensor Tube



Installation and Operation

Instrument Installation

The MC300 is pre configured for immediate installation and use. The unit should be first mounted in the desired location and properly secured. In choosing a location, the display should be clearly visible by an operator and positioned in such a way that the operator can easily make adjustments to the instrument. All wiring should be neatly dressed and bundled with special care not to have any wiring adjacent to AC power distribution. After proper installation of sensors and wiring, the unit can be connected to an AC power source and put into operation.

IT IS RECOMMENDED THAT POWER IS NOT APPLIED TO THE INSTRUMENT DURING THE INSTALLATION OF ANY WIRING AND SENSORS.

Sensor Installation

It is desirable that the thermocouple and cold cathode sensor tubes be mounted on the vacuum system in a VERTICAL POSITION open end extending downward. The 4A convection sensor *MUST* be installed in the VERTICAL POSITION.

The electronic unit is factory calibrated at time of order. To ensure proper operating conditions *it is necessary to use factory-manufactured cables.*

Contamination of thermocouples sensor can be caused by the process occurring in the vacuum vessel, or by pump fluid back streaming and is a critical factor affecting the measurement of high vacuum.

Depending upon the degree of contamination and the accuracy required, it is recommended that sensor be periodically replaced and that filters (with line of sight baffles (P/N 2-2100-50) be used to protect thermocouple sensors.

The thermocouple and convection sensor tubes incorporate a 1/8" National Pipe Thread (1/8" NPT) fitting for connection to the vacuum system and other mounting configurations are available.

The instrument may be turned on at any time, since atmospheric pressure will not harm the thermocouple sensor tube elements or cause overdrive on the metering circuit. A brief 15-minute warm up is required before vacuum measurements can be made within stated tolerances.

Wiring the instrument

Sensor wiring

The MC300 requires sensors & cables (sold separately) for each channel. Certain levels of calibration require a specific cable and sensor be used with channel 1 or 2. In this case the cable and sensor are marked for use as a set and must be used as such. Otherwise the cables can be used with either rough vacuum channel. To ensure measurement integrity and protection from ambient electrical noise, ground lugs are provided on each sensor cable shield. These lugs should be connected to the ground screws provided on the rear panel.

Analog Output Wiring

Provisions are made to connect the instrument to a chart recorder or programmable logic controller. Two different format signals are provided and are described in Section 5 Analog Outputs. In all cases follow the external device manufacturer's instructions for wiring and using these signals. Linear (**LIN**) output is computer generated so that the voltage signal is plotted as a straight line as a function of pressure.

Traditional (**TRDL**) signal is one that represents the non-linear signal that is representative of the actual raw sensor data. The 4A Convection version has **Linear/Decade** and **Linear** outputs. By means of a factory settable internal jumper a full range Traditional signal is available in lieu of the **Linear/Decade** recorder output. Please refer to Section 5 Analog Output (4A) for a summary of the signals available

Relay Contact Wiring (Set point Relays)

There are four set point relays available for use to control ON/OFF or Open/close (binary state) devices. The relays are assignable to any one of the vacuum signal input channels through front panel software control.

There are three connections for each relay. They are NORMALLY CLOSED (NC), COMMON (C) and NORMALLY OPEN (O). The operation mode of each is described as follows.

NORMALLY CLOSED:

In this state there is an electrical continuity path between terminals **C** and **NC**. This continuity path is broken when the software set point values dictates an ON state for the specific measurement channel. Continuity is returned when the OFF state is dictated by software control. In the power off mode of the MC300 (due to failure of the main power source or turning off the instrument), the relay will revert to this state.

NORMALLY OPEN:

In this state there is no electrical continuity path between terminals **C** and **NO**. This Path is established **ONLY** when the Instrument control software satisfies conditions for the ON state. It will break continuity under the instrument control parameters for the OFF condition or the power off mode of the MC300 (due to failure of the main power source or turning off the instrument).

CAUTION:

In utilizing the process relays it is important not to exceed the relay's power handling capacity described in Section 10 Specifications and to fully understand the behavior of the control relay state conditions. Failure to do so will result in premature relay or equipment failure.

Operating the Instrument

This section describes the operation of a properly installed MC300 Instrument

Prior to using the instrument on a vacuum chamber, the unit can be set up in a test mode using simulators to represent the vacuum gauges. This is done to gain familiarity with the unit and to preset relay set points. The following describes operation of the instrument with simulators or vacuum applied to the sensors.

POWER ON:

The instrument is turned on and off by means of a rear mounted power switch. The unit will first display the Software version number and instrument type in a four-digit code. The first two digits refer to the software version and the second two digits refer to the Instrument Sensor type summarized below.

The instrument will then perform a self-diagnosis after which it will begin displaying vacuum measurements. If the unit doesn't pass the self-test, an error code will appear. Pressing the "TEST OP" button can clear the code, but proper operation of the instrument may be curtailed. It is recommended not to use the instrument if the self diagnosis fails. Contact the factory for instructions. Allow a minimum of 15 minutes from an instrument "cold start" for the sensor readings to stabilize.

GAS CORRECTION FACTOR:

The instrument is calibrated for use in Nitrogen (dry air) but the MC300 has the ability to adjust its pressure readings to compensate the thermal conductivity gauges for the use of ARGON as a background gas. When Argon gas is selected, the GAS light will flash during operation of the gauge.

To change the gas correction factor:

- 1) Assure the rear mounted operator **lock out switch** is in the “**OFF**” position (the switch is in the down position)
- 2) Press the **SETUP** button once
- 3) The Nitrogen (N₂) or Argon (Ar) display will flash
- 4) Press the **UP** or **DOWN** arrow buttons to select a gas correction, The flashing display is the gas selected)
- 5) Press the **TEST OP** button to complete the selection

(**Note:** if the **TEST OP** switch is not pressed in 60 seconds the instrument will return to normal operation and the change in gas correction is not accepted)

CHANGE MEASUREMENT UNITS:

The MC300 has the ability to display vacuum values in Pascals, MBAR or MICRONS and TORR.

- 1) Assure the rear mounted operator **lock out switch** is in “**OFF**” position, (the switch is in the down position)
- 2) Press the **SETUP** button once
- 3) Nitrogen (N₂) and Argon (Ar) display will flash
- 4) Press the **SETUP** a second time
- 5) The Pascal, MBAR or TORR lamp will flash
- 6) Press the **UP** or **DOWN** arrow buttons to select the desired unit of measurement
- 7) Press the **TEST OP** button to complete the selection

(**Note:** if the **TEST OP** switch is not pressed in 60 seconds the instrument will return to normal operation and the change in gas correction is not accepted)

ASSIGN SET POINT RELAYS AND VALUES:

The instrument has four relays that are assignable to any of the vacuum measurement channels. Thermocouple (or Convection) Channel 1 is Channel 1 (CH1), thermocouple (or Convection) Channel 2 is Channel 2 (CH2) and the Ion gauge is Channel 3 (CH3). Setpoint SP 1 is relay #1, setpoint SP 2 is relay #2 etc.

- 1) Assure the rear mounted **operator lock out switch** is in the “**OFF**” position, (the switch is in the down position)
- 2) Press the **SETUP** button once
- 3) The **Nitrogen (N2)** or **Argon (Ar)** display will flash
- 4) Press the **SETUP** a second time
The measurement units (PASCAL, MBAR or TORR) lamp will flash
- 5) Press the **SETUP** a third time
- 6) The set point SP 1 will appear in the left display, the channel number CH1, 2 or 3 will appear in the right display
- 7) Use the **UP** or **DOWN** arrows to select the channel number 1,2 or 3
- 8) Press the **SETUP** button again. “**ON**” will appear in the right display, the “**ON**” value will appear in the lower left display
- 9) Press the **UP/DOWN** button to adjust the “**ON**” value. Press and hold the **UP/DOWN** button to rapidly advance the “**ON**” value.
- 10) Press the **SET UP** button again. “**OFF**” will appear in the right display the relay “**OFF**” value will appear in the lower left display
- 11) Press the **UP/DOWN** buttons to adjust the “**OFF**” value. Press and hold the **UP/DOWN** button to rapidly advance the “**OFF**” value.
- 12) Press the **SET UP** button again and the next relay, SP 2 will appear. The sequence listed in steps 6 and 11 are repeated until all four relays have been assigned.

The MC300 will return to its normal operating mode after the fourth relay has been set up or 60 seconds have elapsed since the last button press. Changes are stored after the complete set up of an individual relay channel. These set up parameters are stored in Non volatile memory and are not lost during Power outages.

NOTE: *Set point changes are also accepted by the MC300 by pressing the “TEST OP” button at any point in the set up. The Instrument will not accept “OFF” values that are lower than the “ON” value. “ON” values entered that are greater than the “OFF” values will automatically change the “OFF” value one unit higher than “ON”.*

Analog Recorder Outputs

- 0-10VDC analog recorder output voltage/pressure conversions are provided for each type of Sensor in the figures 5 & 6.
- These voltage signals are available at the rear panel of the MC300. See figure 2 for locations of the connections.
- Outputs #1 and #2 are for thermocouple or convection sensors. These outputs are 0-10 volts and are available in a traditional or linear format. See figures 5 or 6.

MICRONS ARGON READS	TRAD'L REC OUT VOLTS	LIN REC OUT OUT
(-5)	10.59	-0.05
(-1)	10.16	-0.01
0	10.00	0.00
1	9.84	0,01
5	9.41	0.05
10	8.92	0.10
20	8.03	0.20
30	7.23	0.30
40	6.63	0.40
50	6.13	0.50
60	5.69	0.60
70	5.31	0.70
80	4.95	0.80
90	4.63	0.90
100	4.37	1.00
150	3.37	1.50
200	2.89	2.00
300	2.23	3.00
400	1.88	4.00
500	1.67	5.00
600	1.58	6.00
700	1.50	7.00
800	1.42	8.00
900	1.34	9.00
1000	1.26	10.00
2000	1.02	10.20
5000	0.92	10.20
10000	0.90	10.20
20000	0.88	10.20
CABLE	0.00	10.20

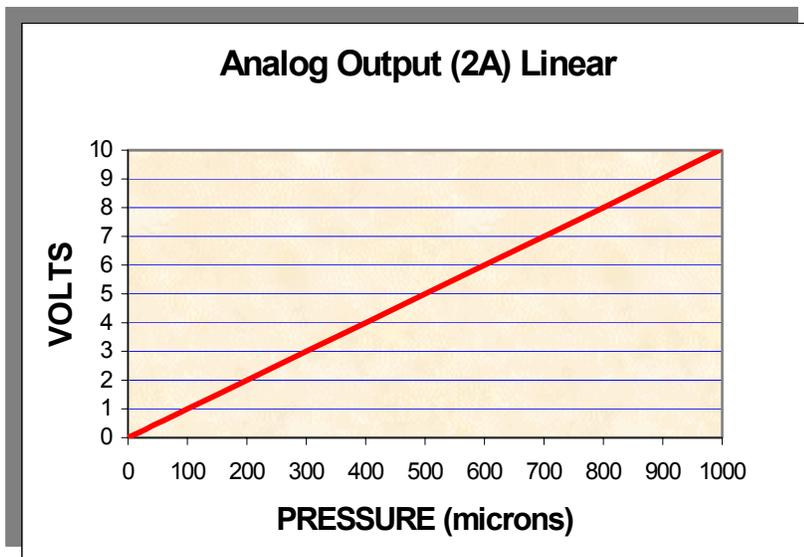


Figure 5
Analog Output (2A)

TORR/ MICR ARG READS	TRDL OUT	L/D REC OUT 1 VOLT/ DEC	LIN OUT VOLTS
(-5)-OL'D	-0.065	3.500	<-.050
(-1)	-0.013	3.900	-.010
0-	0.000	4.000	0.000
1 u	0.013	4.100	0.010
5 u	0.065	4.500	0.050
10 u	0.124	5.100	0.100
20 u	0.238	5.200	0.200
30 u	0.344	5.300	0.300
40 u	0.450	5.400	0.400
50 u	0.546	5.500	0.500
60 u	0.638	5.600	0.600
70 u	0.730	5.700	0.700
80 u	0.816	5.800	0.800
90 u	0.898	5.900	0.900
100 u	0.980	6.100	1.000
150 u	1.350	6.150	1.500
200 u	1.670	6.200	2.000
300 u	2.285	6.300	3.000
400 u	2.630	6.400	4.000
500 u	2.992	6.500	5.000
800 u	3.824	6.800	8.000
1 T	4.226	7.100	10.000
2 T	5.440	7.200	13.500
3 T	6.080	7.300	"
4 T	6.440	7.400	"
5 T	6.772	7.500	"
10 T	7.412	8.100	"
20 T	7.782	8.200	"
30 T	7.910	8.300	"
40 T	7.936	8.400	"
50 T	7.976	8.500	"
60 T	8.006	8.600	"
80 T	8.042	8.800	"
100 T	8.072	9.100	"
120 T	8.124	9.120	"
150 T	8.180	9.150	"
160 T	8.224	9.160	"
170 T	8.256	9.170	"
180 T	8.280	9.180	"
200 T	8.328	9.200	"
300 T	8.756	9.300	"
400 T	9.208	9.400	"
500 T	9.544	9.500	"
600 T	9.772	9.600	"
760 T	10.000	9.760	"
900 T	10.142	9.90	"
1000 T	10.232	10.000	"
CABLE	>10.5	10.11	"

Figure 6
Analog Output (4A)

If L/DOUT = INT .DDD Volts

TORR = 0.DDD x 10 EXP (INT -6)

If .DDD < 0.1, use 0.1

Maintenance

The vacuum measuring sensors, if installed properly, require very little maintenance under normal operating conditions.

If the unit should cease to operate properly, certain checks can be made:

1. If a sensor tube simulator is available, it can be used. The sensor tube simulators are designed to be used as a check to see if the cable and the electronics are working properly.

The simulators are marked for use with the various sensors. Although no maintenance is required to keep the tube simulator in working condition, a periodic check should be done against a calibrated standard unit.

To use the simulator, turn off and disconnect the cable from the sensor tube and plug the sensor tube simulator in its place. Turn power on and check the output voltage, it should correspond to the pressure that is written on the sensor tube simulator's label.

2. If you do not have a tube simulator, it is still possible to check the operation of the instrument if you are able to reduce the system pressure to 10⁻⁵ Torr. At this pressure, the thermocouple and the convection sensors should display zero and give Analog output of zero volts. The "ZERO" adjust trimmers at the rear panel can be used to set up the zero readings. If output still appears to respond incorrectly, a new sensor tube should be replaced to restore the assembly to proper operation.
3. The following table summarizes the messages on the MC300 display under several different operating conditions as well as the expected Analog outputs.

2A			
<u>Display</u>	<u>Conditions</u>	<u>Traditional Analog Output (Volts)</u>	<u>Linear Analog Output (Volts)</u>
-OLd	<-1 micron	+10.59	-0.05
-1	Incorrect ZERO adjust	+10.16	-0.01
0 microns	Lowest Reading	+10.00	0.00
20 Torr	Highest Reading	+0.88	+10.20
CabL	> 20 Torr	+0.00	+10.20

4A				
<u>Display</u>	<u>Conditions</u>	<u>Traditional Recorder Output Fact Option (Volts)</u>	<u>Linear Decade Analog Output (Volts)</u>	<u>Linear Analog Output (Volts)</u>
-OLd	<-5 microns	-0.07	+3.50	<-.05
-1	Incorrect ZERO adjust	-0.01	+3.90	-0.01
0 microns	Lowest Reading	0.00	+4.00	0.00
990 Torr	Highest Reading	+10.23	+9.99	+13.50
CAbL	>990 Torr	>+10.50	+10.11	+13.50

CHAPTER 7

Calibration

All TELEVAC instrumentation is calibrated at the factory. No further calibration at the customer's facility should be required.

For a reliable re-calibration at a later date, it is necessary to have a reference standard vacuum system whose pressure is known very accurately. For such a calibration, the instrument, sensor tube and cable should be returned to TELEVAC for re-certification.

However, if the vacuum calibration certification is to be done at the customer's facility, equipment of certifiable accuracy should be used by a knowledgeable electronics technician trained in vacuum calibration.

Calibration Verification

1. Connect sensor to the known vacuum source.
2. Plug unit into 115VAC. Allow a minimum of 15 minutes warm-up.
3. Pump the system down to high vacuum. At 10⁻⁵ TORR verify that the thermocouple or convection gauge reads at “0” VDC. If not, adjust the “zero” potentiometer.
4. Make a comparison table of indicated pressure on the instrument to that of the reference vacuum standard. The comparisons should be made typically at “0” (red line), 10, 100 and 1,000 millitorr and at 1, 10, 100, 500 and 760 Torr, (depending on the 2A or 7A gauge type).


Troubleshooting

Troubleshooting of the circuit or components is similar to any industrial electrical equipment, i.e., checking for circuit continuity, shorts, grounds, resistors, values, etc.

Generally, those familiar with electrical equipment should have no difficulty location faults in either gauge or electronics unit by systematically proceeding through the circuit. The enclosed diagram should facilitate maintaining the instrument. In order to troubleshoot the unit, your gauge tube and cable must be in working condition and plugged into the unit.

NOTE: If, after doing some or all of the above, the unit is still inoperative, return to factory for repair.

Dimensions

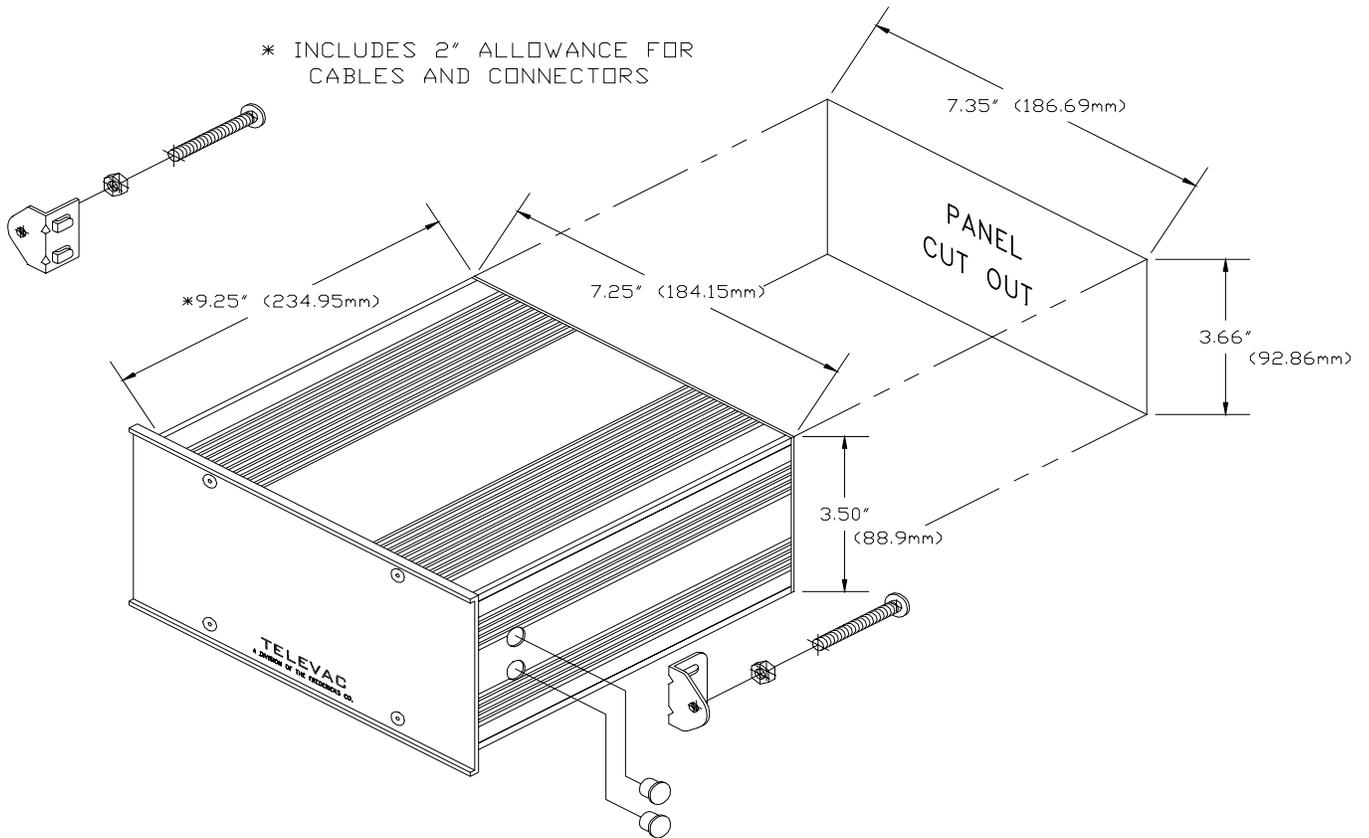

HOLE PLUGS MAY BE REMOVED
IF CUSTOMER REQUIRES BRACKETS

<u>FRONT PANEL</u>	<u>MM</u>	<u>INCHES</u>
Height	102	4.0
Width	197	7.75
<u>UNIT</u>		
Height	88.9	3.5
Width	184.15	7.25
<u>DEPTH</u>		
Excluding connectors	197	7.75
Including connectors (approx.)	234.95	9.25
<u>PANEL CUT OUT</u>		
Height	92.86	3.66
Width	186.69	7.35

Specifications

<u>Range</u>	<u>Power</u>
See table in Chapter 1	115 VAC, 230 VAC (optional)
<u>Calibration Medium</u>	<u>Oper. Temp.</u>
Dry air, (or nitrogen)	+15 ° to +50° C
<u>Frequency</u>	<u>Fuse</u>
60 Hz or 50 Hz	Internal
<u>Display/Output</u>	<u>Relay Contacts</u>
Digital/analog	5 Amps @ 230 VAC
3 digits, 0-10 Volts	
<u>Weight (instrument)</u>	
5 lbs. Max. exclusive of sensors and cables	

Unpacking and Inspection

Before each unit is installed or operated, a quick inspection should be performed and the following noted:

- ◆ Damage to the unit (scratches, nicks, dent, cracks...)
- ◆ Missing (screws, switches or switch hardware)
- ◆ Broken barrier strips...
- ◆ Broken or loose components within instrument

**Should any of the above problems be encountered, contact the factory immediately.
Any unauthorized repairs will void the warranty.**

Warranty Information

- The Fredericks Company warrants all instruments and components of its manufacture to be free of defects in materials and workmanship.
- Our obligation under this warranty is limited to servicing or adjusting any instrument returned to us and replacing any part, except those specifically exempt from this guarantee, which shall within one year after delivery to the original purchaser be returned to us with transportation charges prepaid, and which our examination should disclose to our satisfaction to have been defective. Those portions specifically exempt from this guarantee are gauge tubes, batteries as well as meters, which have been disassembled or physically damaged.
- The Fredericks Company does not assume any other obligation than that stated in this warranty nor does it authorize any person to assume for them any liability in connection with the sale, service or use of the Fredericks Company's instruments.

Ordering Information

SPECIFY 110-VOLT OR 220-VOLT OPERATION – UNIT SHIPPED 110 VOLT STANDARD

<u>MODEL</u>	<u>PART NUMBER</u>	<u>SENSORS</u>	<u>CABLES</u>
MC300 2A	2-4503-401	2A	2A
MC300 4A	2-4503-402	4A	4A

2A THERMOCOUPLE



- √ Measurement Range—1 to 20,000 microns
- √ Construction—Nickel-Plated Brass, Stainless Steel

<u>Model</u>	<u>Part Number</u>
2A 1/8" NPT Nickel Brass	2-2100-10
2A 1/8" NPT Stainless Steel	2-2126-001
2a NW 16 KF Stainless Steel	2-2126-030

Other fittings available- call factory

4A CONVECTION



- √ Measurement Range-10-3 TORR to Atmosphere
- √ Construction-Nickel-Plated Brass, Stainless Steel

<u>Model</u>	<u>Part Number</u>
4A 1/8" NPT Nickel Brass	2-2119-001
4A 1/8" NPT Stainless Steel	2-2120-001
4A NW 16 KF Stainless Steel	2-2120-030

Other fittings available-call factory

2A/4A cable



2A Cable

4A Cable

10 Foot	2-9800-077	2-9820-010
20 Foot	2-9800-078	2-9820-020
35 Foot	2-9800-079	2-9820-035
50 Foot	2-9800-080	2-9820-050

ACCESSORIES

- | | |
|---------------------------------------|------------|
| √ Mounting Ear Kit (INCLUDED) | 6-2700-60 |
| √ Zero Micron 2A Simulator | 2-2100-237 |
| √ Zero Micron 4A Simulator | 2-2119-000 |
| √ Filters for 1/8" NPT 2A/ 4A Sensors | 2-2100-50 |