

VARIAN




vacuum technologies

***Turbo-V60
Leak Detector
PCB Controller***

Model 969-9840

(GB) INSTRUCTION MANUAL

***Turbo-V 60 Leak Detector
PCB Controller***

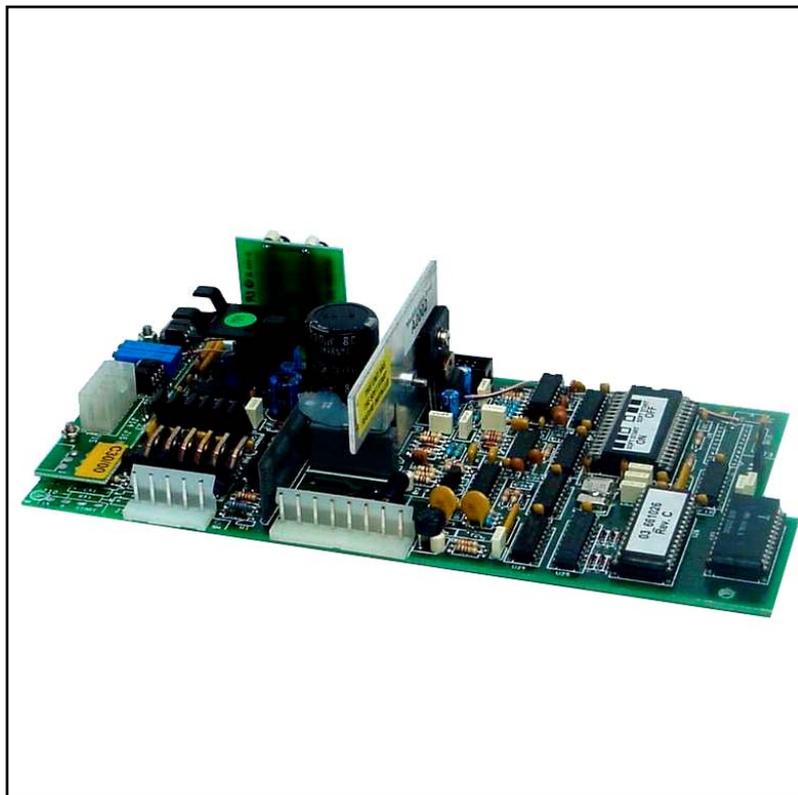



Dear Customer,


Thank you for purchasing a VARIAN vacuum product. At VARIAN Vacuum Technologies we make every effort to ensure that you will be satisfied with the product and/or service you have purchased.

As part of our Continuous Improvement effort, we ask that you report to us any problem you may have had with the purchase or operation of our product. On the back side you find a Corrective Action Request form that you may fill out in the first part and return to us.

This form is intended to supplement normal lines of communications and to resolve problems that existing systems are not addressing in an adequate or timely manner.

Upon receipt of your Corrective Action Request we will determine the Root Cause of the problem and take the necessary actions to eliminate it. You will be contacted by one of our employees who will review the problem with you and update you, with the second part of the same form, on our actions.

Your business is very important to us. Please, take the time and let us know how we can improve.

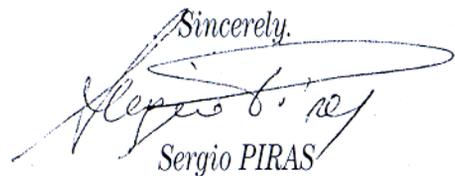Sincerely,

Sergio PIRAS

*Vice President and General Manager
VARIAN Vacuum Technologies*

Note: Fax or mail the Customer Request for Action (see backside page) to VARIAN Vacuum Technologies (Torino) - Quality Assurance or to your nearest VARIAN representative for onward transmission to the same address.

CUSTOMER REQUEST FOR CORRECTIVE / PREVENTIVE / IMPROVEMENT ACTION

TO : VARIAN VACUUM TECHNOLOGIES TORINO - QUALITY ASSURANCE

FAX N° : XXXX - 011 - 9979350

ADDRESS: VARIAN S.p.A. - Via F.lli Varian, 54 - 10040 Leinì (Torino) - Italy

E-MAIL : marco.marzio@varianinc.com

NAME _____	COMPANY _____	FUNCTION _____
<p>ADDRESS : _____</p> <p>TEL. N° : _____ FAX N° : _____</p> <p>E-MAIL : _____</p>		
<p>PROBLEM / SUGGESTION :</p> <p>_____</p> <p>_____</p> <p>_____</p> <p>_____</p>		
<p>REFERENCE INFORMATION (model n°, serial n°, ordering information, time to failure after installation, etc.) :</p> <p>_____</p> <p>_____</p> <p>_____</p> <p style="text-align: right;">DATE _____</p>		

<p>CORRECTIVE ACTION PLAN / ACTUATION (by VARIAN VTT)</p> <p>_____</p> <p>_____</p> <p>_____</p> <p>_____</p> <p>_____</p>	<p>LOG N° _____</p>
--	---------------------

XXXX = Code for dialing Italy from your country (es. 01139 from USA; 00139 from Japan, etc.)



TABLE OF CONTENTS

Section		Page
-	Safety summary	1
I	Description	
1-1	General	2
1-2	Turbo-V60 controller description	2
1-3	Controller specifications	3
1-4	Controller outline	3
II	Installation	
2-1	General	4
2-2	Line voltage selection	4
2-3	Power interconnections	4
2-4	Input/Output interconnections	5
2-5	Turbo-V pump connection	5
III	Operation	
3-1	General	6
3-2	Start-up	6
3-3	Soft Start mode deselection	6
3-4	Starting the pump	6
3-5	Pump shutdown	7
3-6	Power failure	7
IV	Maintenance	
4-1	General	8
4-2	Controller test	8

SAFETY SUMMARY

Operators and service personnel must be aware of all hazards associated with this equipment. They must know how to recognize hazardous and potentially hazardous conditions, and know how to avoid them. The consequences of unskilled, improper, or careless operation of the equipment can be serious. This product must only be operated and maintained by trained personnel. Every operator or service person must read and thoroughly understand operation/maintenance manuals and any additional information provided by Varian.

All warnings and cautions should be read carefully and strictly observed. Address any safety, operation, and/or maintenance questions to your nearest Varian office.

The following format is used in this manual to call attention to hazards:



Warnings are used when failure to observe instructions or precautions could result in injury or death.



Cautions are used when failure to observe instructions could result in damage to equipment, whether Varian supplied or other associated equipment.

NOTE

Information to aid the operator in obtaining the best performance from the equipment.

1-1 General

The Turbo-V60 Leak Detector PCB controller is a microprocessor-controlled, solid-state, frequency converter with self-diagnostic and protection features.

The controller drives (within ten steps) the Turbo V-60 pump during the starting phase by controlling the voltage and current respect to the speed reached by the pump.

It incorporates all the facilities required for the automatic operation of the Turbo-V60 pump series. Remote start/stop and output control capability are provided via auxiliary connectors.

1-2 Turbo-V60 controller description

The controller is a solid-state frequency converter which is driven by a single chip microcomputer. The package composition is:

- Power transformer with interconnection cables
- PCB including: power supply and 3-phase output, analog and input/output section, microprocessor and digital section
- Controller to pump interconnection cable.

The power supply and the 3-phase output converts the single phase (50-60 Hz) AC mains supply into a 3-phase, low voltage, medium frequency output which is required to power the Turbo-V pump.

The microcomputer generates the variable output frequency and controls the 3-phase output voltage according to the software and the gas load condition of the pump.

Moreover, it manages input and output signals for a fully automatic operation.

A dedicated non-volatile RAM is used to store pump operating parameters and the input/output programmed information upon failure for a period of 10 years accumulated off time.

Two adjustable trimmers are provided to set the pump rotational speed as follows:

- P1 – High speed trimmer: 50 to 70 KRPM
- P2 – Low speed trimmer: 30 to 50 KRPM

The controller can be operated via remote signals through input/output connector.

1-3 Controller specifications

Input: Voltage	Two ranges selectable on a three pin connector on the transformer primary: - 120 Vac±20%, - 220 Vac±20%, 1-phase
Frequency	47 to 63 Hz
Power	350 VA maximum
Output: Voltage	54 Vac nominal ±10%, 3-phase
Frequency	1167 Hz, ±2%
Power	150 W maximum
Operating temperature	0°C to + 40 °C
Storage temperature	-20°C to + 70°C
J2 optoisolator input	4 to 12 Vdc
J2 optoisolator output	ICsat 1.6 mA VCE max 0.6 V VCEO 70 V
Interconnecting cables	Pump cable (5-wire, 55 cm long)
Weight	0.5 Kg (1.1 lbs)

1-4 Controller outline

The outline dimensions for the Turbo-V60 Leak Detector PCB controller are shown in Fig. 1-1.

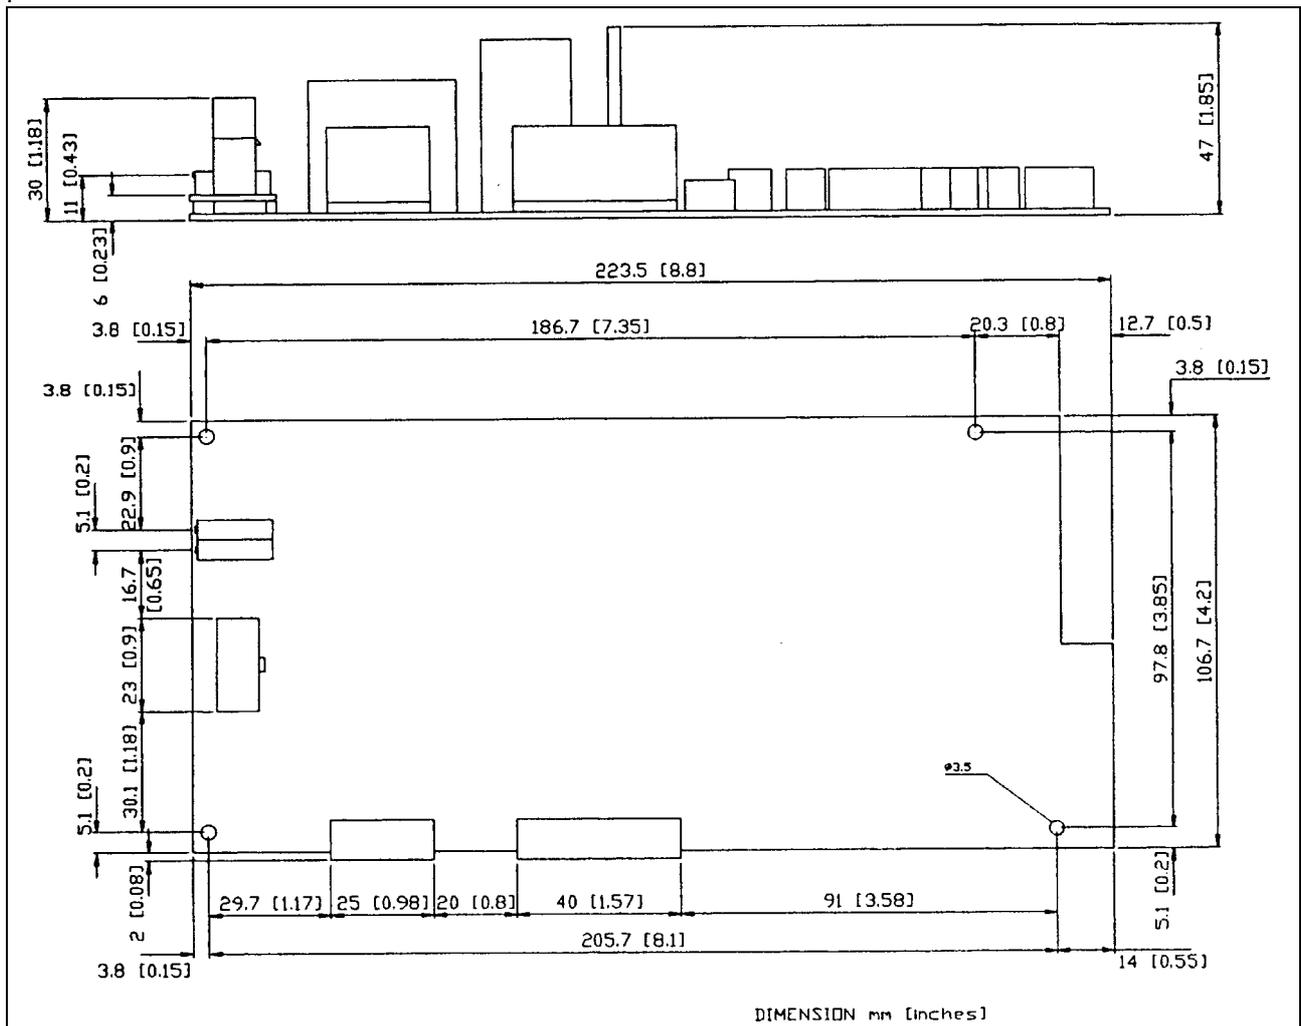


Figure 1-1 – Controller outline

2-1 General

Inspect the controller for any shipping damage.



WARNING!

High voltage developed in the controller can cause severe injury or death. Before servicing the unit, disconnect the input power cable.

NOTE

The PCB installed into the customer system must be positioned so that cold air (forced or natural convection) can flow through the PCB components

2-2 Line voltage selection

The controller can operate with two ranges of input voltage:

- 120 Vac \pm 20%
- 220 Vac \pm 20%

The line voltage selection is done on the three pin male connector on the primary wires of the transformer:

- for 120 Vac connect the line wires as follows:
 - 120 Vac to pin 2 (white)
 - 0 V to pin 3 (bleu)
- for 220 Vac connect the line wires as follows:
 - 220 Vac to pin 1 (brown)
 - 0 V to pin 3 (bleu)

NOTE

The mating connector and the female pins are provided

2-3 Power interconnections

The power supply from the external transformer must be connected to J8 connector

See Fig. 2-1 for interconnections detail.

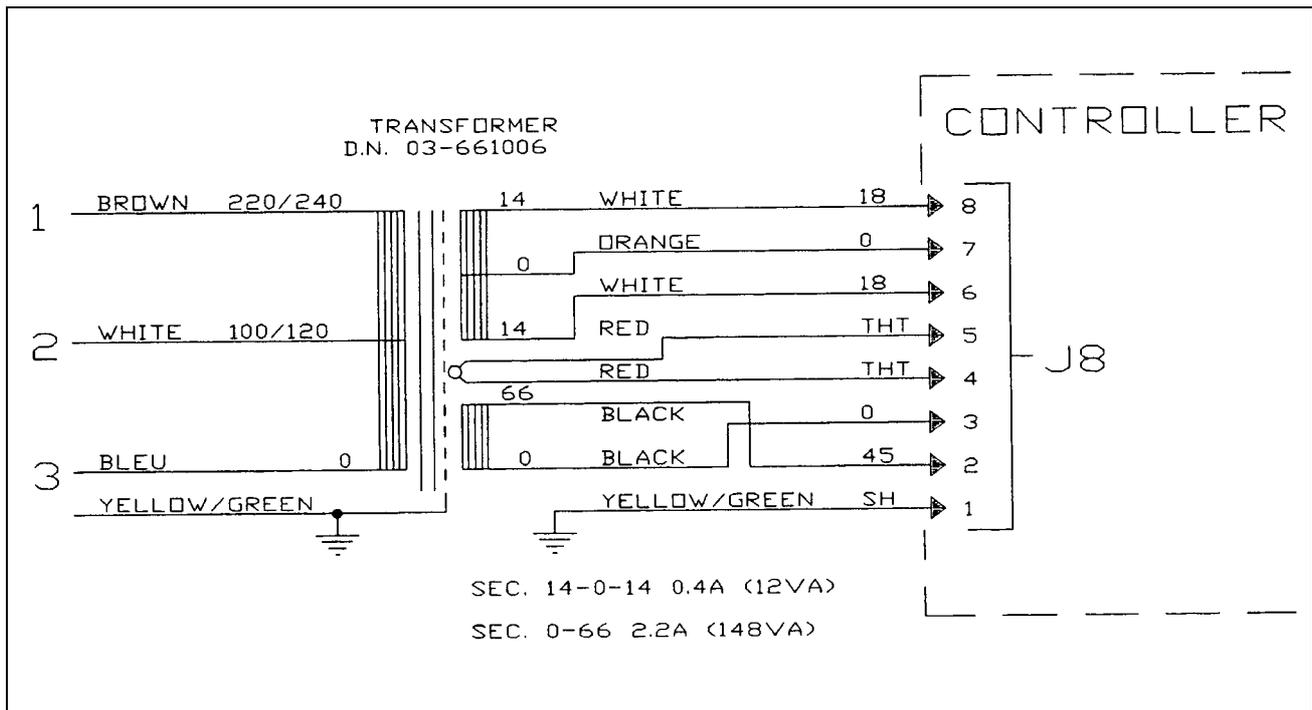


Figure 2-1 - J8 connector interconnections

2-4 Input/Output interconnections

All the input/output signals to the controller must be connected at J15 mating connector (see Fig. 2-2).

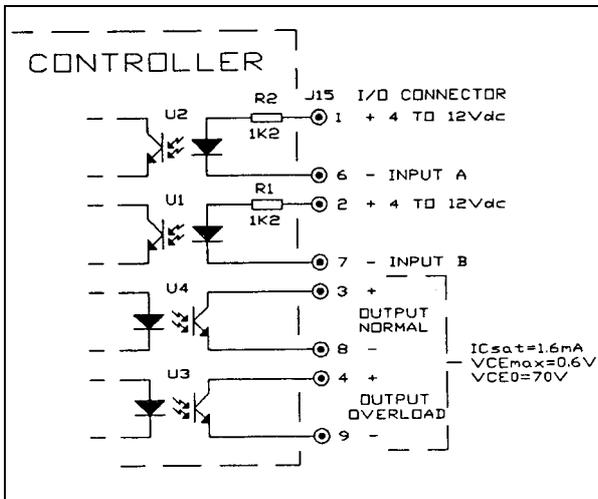


Figure 2-2 – Input/Output connector

Pin 1-6 Input A optically isolated from the internal circuit.

In conjunction with the Input B determines the controller mode of operation according to the following truth table.

Pin 2-7 Input B optically isolated from the internal circuit.

In conjunction with the Input A determines the controller mode of operation according to the following truth table.

INPUT SIGNAL LOGIC LEVEL		CONTROL UNIT CONDITION
A	B	
LOW	LOW	LOW FREQUENCY
LOW	HIGH	HIGH FREQUENCY
HIGH	LOW	HIGH FREQUENCY
HIGH	HIGH	LOW FREQUENCY

Pin 3-8 Output Normal optically isolated from the internal circuit.

Pin 4-9 Output Overload optically isolated from the internal circuit.

2-5 Turbo-V pump connection

A 55 cm long cable is provided to connect the controller to the pump.

Figure 2-3 shows the pump output connector configuration where pins:

Pins A-F = pump temperature sensor

Pins B-C-D = 54 Vac 3-phase output to pump motor stator

Pin E = ground.

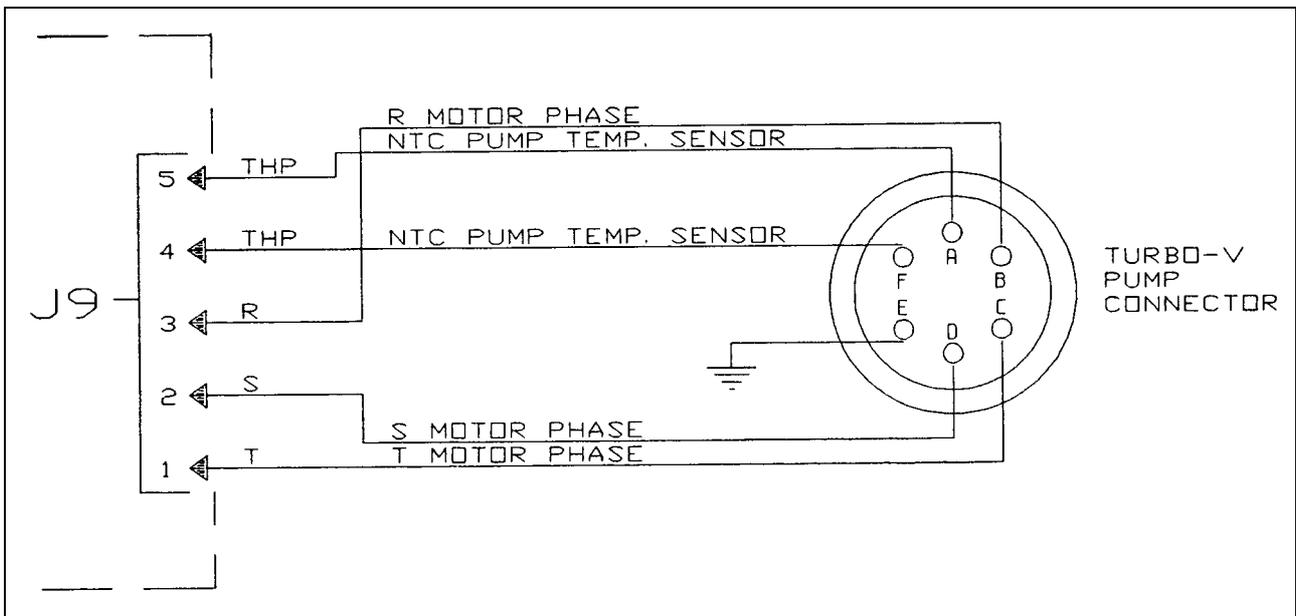


Figure 2-3 – Turbo-V pump connector

3-1 General

Make all vacuum manifold and electrical connections and refer to Turbo-V pump instruction manual prior to operating the Turbo-V controller.



WARNING!

To avoid injury to personnel and damage to the equipment, if the pump is laying on a table make sure it is steady. Never operate the Turbo-V pump if the pump inlet is not connected to the system or blanked off.

The controller operates completely automatically after the remote start command is given.

The only user available commands are two trimmers to set the pump rotational speed: the first one (P1) sets the high speed, the second (P2) sets the low speed.

The two trimmers are factory preset as follows:

- P1 (high speed) to 60 KRPM
- P2 (low speed) to 33 KRPM

To select different rotational speeds, act on the appropriate trimmer. The variation ranges are:

- P1: 50 to 70 KRPM
- P2: 30 to 50 KRPM

3-2 Startup

Plug the controller power cable into a suitable power source.

The controller is factory preset with the Soft Start mode enabled that allows the pump to ramp-up to Normal speed slowly with a minimum ramp-up time of 75 seconds and a maximum of about 45 minutes.

If it is necessary to deselct this mode refer to paragraph 3-3.

If the Soft Start mode is deselected, the ramp-up will be done within 60 seconds.

3-3 Soft Start mode deselection

The Soft Start mode is enabled and disabled by means of a jumper located on the controller PCB.

To deselect the Soft Start mode operate as follows:

- Disconnect the power from the controller.
- Move the red jumper from the actual position to the other according to the label attached over the integrated circuit near the jumper (see Fig. 3-1).
- Connect the power.

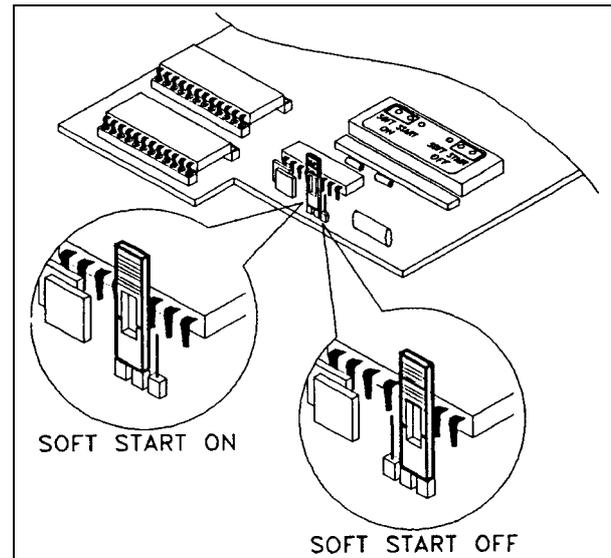


Figure 3-1- Soft Start jumper

3-4 Starting the pump

To start the pump it is necessary to set the Input A and Input B signals on J15 connector both to low logic level, or one to low and the other to high logic level.

In the first case the output to the pump is at low frequency, in the other case the output is at high frequency.

The time to change the speed from low frequency (33 KRPM) to high frequency (60 KRPM) is 12 sec.

The time to change from high frequency (60 KRPM) to low frequency (33 KRPM) is 3 sec.

3-5 Pump shutdown

To shutdown the pump it is necessary to set the Input A and Input B signals on J15 connector both to high logic level.

3-6 Power failure

In the event of a power failure (momentary or long term), the Turbo-V controller will stop the turbopump.

When power is restored, the Turbo-V controller automatically restarts the turbopump.

4-1 General

Replacement controllers are available on an advance exchange basis through Varian. If necessary, information is provided to aid the operator in determining malfunctions and corrective steps to be taken.



WARNING!

Voltages developed in the unit are dangerous and may be fatal. Service must be performed by authorized personnel only.

4-2 Controller test

a) Equipment required

- Digital voltmeter (DVM) true RMS.
- Dummy load: 3 x 48Ω, 50W each or 3 x 78Ω, 50W each.
- Potentiometer 50KΩ, 1/4W minimum.

b) Test set up

- Remove the power cable.
- Disconnect the Turbo-V controller.
- Set potentiometer to 30KΩ and connect it as directed in Fig. 4-1.

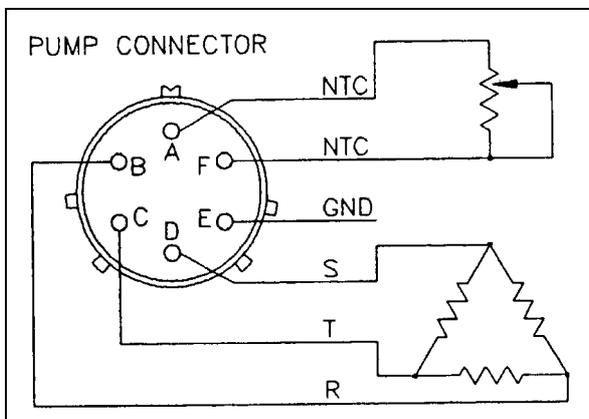


Figure 4-1 – Dummy load connections

4-2.1 Power supply test

a) DC voltage test

Check the DC voltages referring to test points indicated in Fig. 4-2. Refer also to Figg. 4-3 and 4-4. The meter should read:

- + 5Vdc \pm 5%
- \pm 12 Vdc \pm 5%
- Ground reference = case of Q3.

Switch on the controller and check:

- 54 Vdc \pm 10% between TP3(-) a TP5(+) (Fig. 4-2).

b) AC three-phase output voltage test

On the pump connector connect the DVM in turn between: pins B and C, B and D, C and D.

The meter should read 44 Vac \pm 15%; a different value of 0.4 Vac is tolerable between phase and phase.

4-2.2 Test with dummy load

- Connect the 48Ω or the 78Ω dummy loads to the pump connector pins B, C, D as shown in Fig. 4-1.
- Disconnect the potentiometer, set it to 10KΩ, and then reconnect it.
- Connect the power cable.
- Switch on the controller and check the values as per the following table.

	During start-up without Soft Start mode		After start-up	
	With 48Ω dummy load	With 78Ω dummy load	With 48Ω dummy load	With 78Ω dummy load
Current ±10%	1.62 A	1.1 A	1 A	1 A
Power ±10%	80 W	58 W	30 W	48 W
Speed ±4KRPM	17	70	40	63
Temperature ±2°C	52° C	52° C	52° C	52° C

- Check the 3-phase ac output voltage. After start up it should be:
36 Vac with 78Ω dummy load and
21 Vac with 48Ω dummy load.

Switch off the controller and remove the power cable.

4-2.3 Pump over-temperature test

- Disconnect the potentiometer, set it to 5KΩ, and then reconnect it.
- Disconnect the dummy loads.
- Connect the power cable.
- Switch on the controller.
- Check the 3-phase ac output voltage. It should be zero.
- Switch off the controller and remove power cable.

4-2.4 Functional test


Perform the functional test with the turbo-pump, taking care to check the ramp sequence and start up time.


DISPOSAL

Meaning of the "WEEE" logo found in labels
The following symbol is applied in accordance with the EC WEEE (Waste Electrical and Electronic Equipment) Directive.

This symbol (**valid only in countries of the European Community**) indicates that the product it applies to must NOT be disposed of together with ordinary domestic or industrial waste but must be sent to a differentiated waste collection system.

The end user is therefore invited to contact the supplier of the device, whether the Parent Company or a retailer, to initiate the collection and disposal process after checking the contractual terms and conditions of sale.



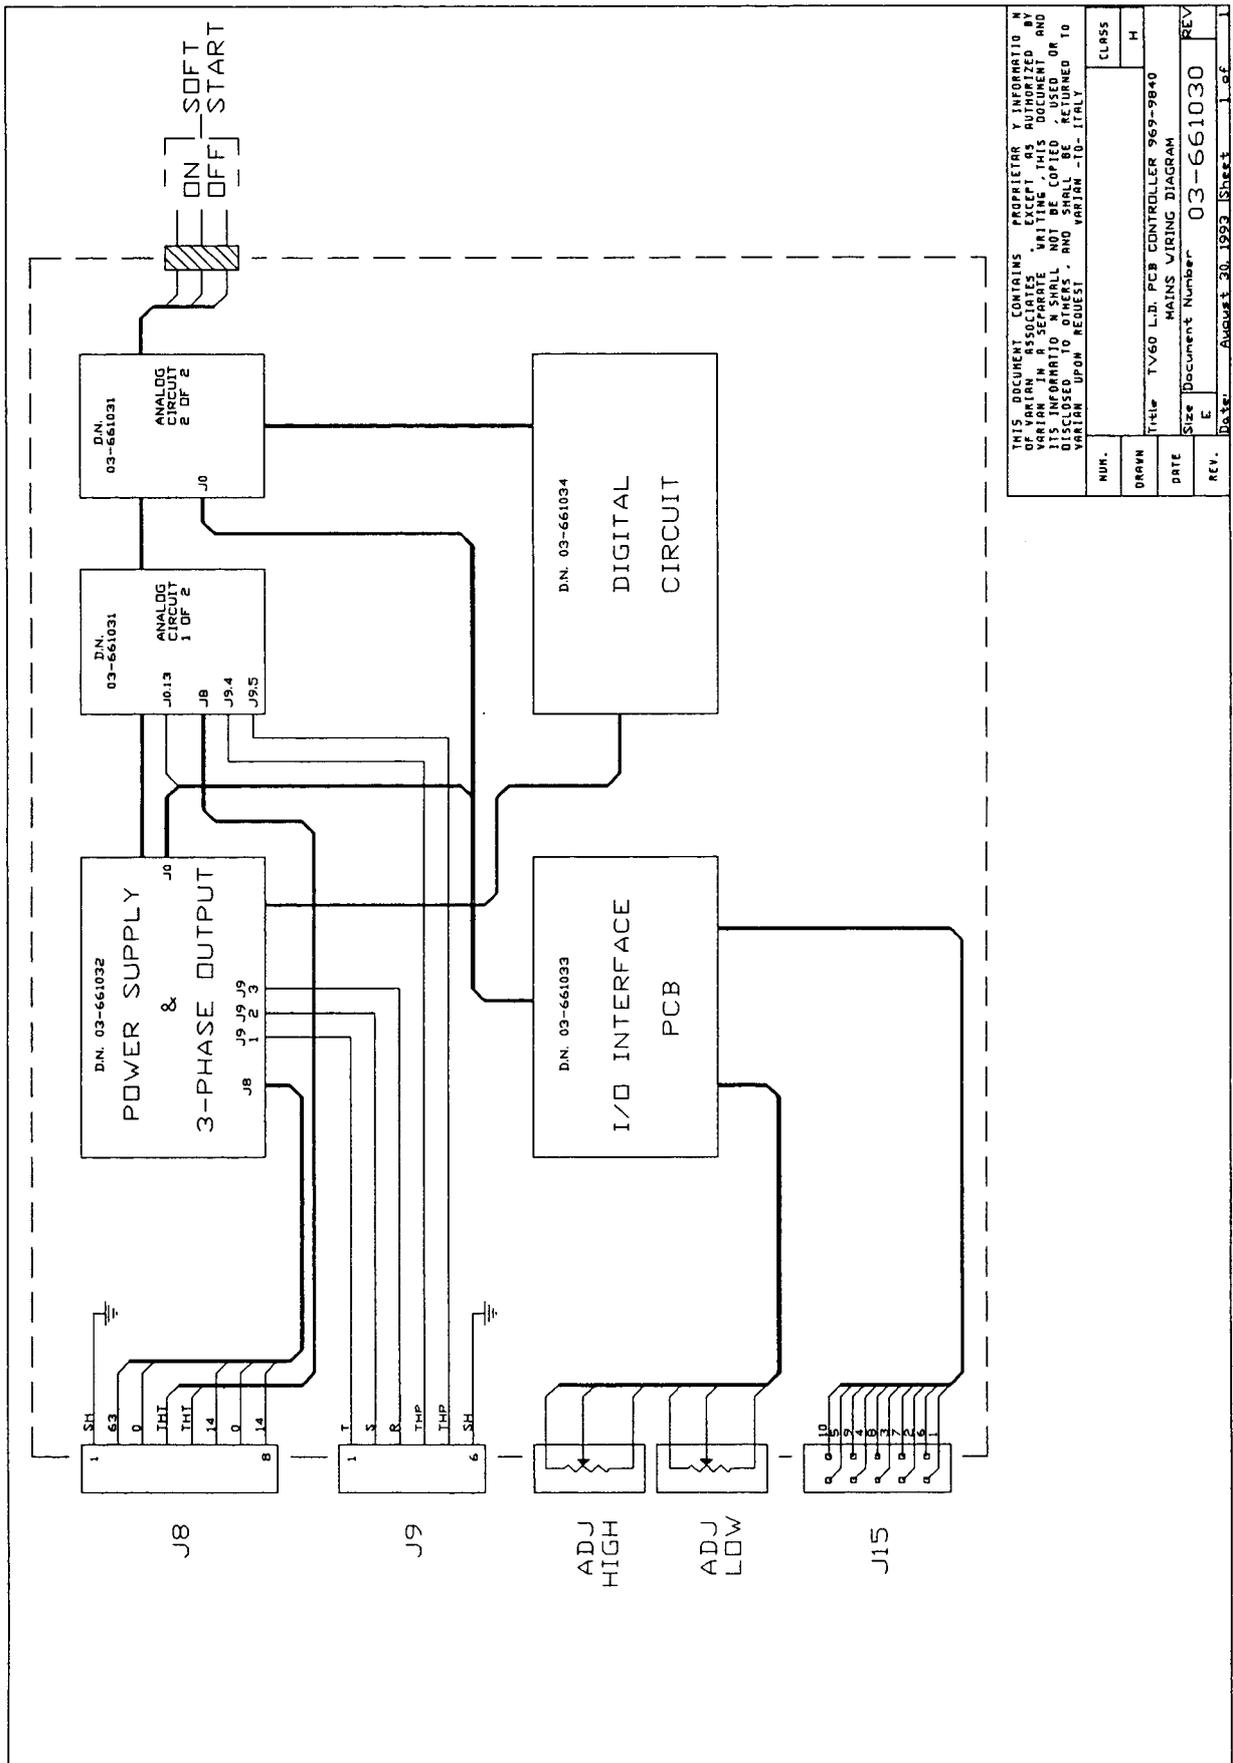

THIS DOCUMENT CONTAINS PROPRIETARY INFORMATION AND IS UNCLASSIFIED EXCEPT WHERE SHOWN OTHERWISE. THIS DOCUMENT AND ITS INFORMATION SHALL NOT BE COPIED, USED OR DISCLOSED TO OTHERS, AND SHALL BE RETURNED TO WARRIOR UPON REQUEST. WARRIOR -10-11714

NUM.	CLASS
DRAWN	H
DATE	
REV.	

Title: TV60 L.D. PCB CONTROLLER 969-9840
 Size: Document Number: 03-661030
 Date: August 30, 1993 Sheet 1 of 1

Figure 4-1



Request for Return



1. A Return Authorization Number (RA#) **WILL NOT** be issued until this Request for Return is completely filled out, signed and returned to Varian Customer Service.
2. Return shipments shall be made in compliance with local and international **Shipping Regulations** (IATA, DOT, UN).
3. The customer is expected to take the following actions to ensure the **Safety** of workers at Varian: (a) Drain any oils or other liquids, (b) Purge or flush all gasses, (c) Wipe off any excess residues in or on the equipment, (d) Package the equipment to prevent shipping damage, (for Advance Exchanges please use packing material from replacement unit).
4. Make sure the shipping documents clearly show the RA# and then return the package to the Varian location nearest you.

North and South America

Varian Vacuum Technologies
 121 Hartwell Ave
 Lexington, MA 02421
 Phone : +1 781 8617200
 Fax: +1 781 8609252

Europe and Middle East

Varian SpA
 Via Flli Varian 54
 10040 Leini (TO) – ITALY
 Phone: +39 011 9979111
 Fax: +39 011 9979330

Asia and ROW

Varian Vacuum Technologies
 Local Office

CUSTOMER INFORMATION

Company name:	
Contact person: Name:	Tel:
Fax:	E-Mail:
Ship Method:	Shipping Collect #: P.O.#:
<i>Europe only:</i> VAT reg. Number:	<i>USA only:</i> <input type="checkbox"/> Taxable <input type="checkbox"/> Non-taxable
Customer Ship To:	Customer Bill To:
.....
.....

PRODUCT IDENTIFICATION

Product Description	Varian P/N	Varian S/N	Purchase Reference

TYPE OF RETURN (check appropriate box)

<input type="checkbox"/> Paid Exchange	<input type="checkbox"/> Paid Repair	<input type="checkbox"/> Warranty Exchange	<input type="checkbox"/> Warranty Repair	<input type="checkbox"/> Loaner Return
<input type="checkbox"/> Credit	<input type="checkbox"/> Shipping Error	<input type="checkbox"/> Evaluation Return	<input type="checkbox"/> Calibration	<input type="checkbox"/> Other

HEALTH and SAFETY CERTIFICATION

Varian Vacuum Technologies **CAN NOT ACCEPT** any equipment which contains **BIOLOGICAL HAZARDS** or **RADIOACTIVITY**. Call Varian Customer Service to discuss alternatives if this requirement presents a problem.

The equipment listed above (check one):

HAS NOT been exposed to any toxic or hazardous materials

OR

HAS been exposed to any toxic or hazardous materials. In case of this selection, check boxes for any materials that equipment was exposed to, check all categories that apply:

Toxic Corrosive Reactive Flammable Explosive Biological Radioactive

List all toxic or hazardous materials. Include product name, chemical name and chemical symbol or formula.

.....

Print Name: Customer Authorized Signature:

Print Title: Date:/...../.....

NOTE: If a product is received at Varian which is contaminated with a toxic or hazardous material that was not disclosed, **the customer will be held responsible** for all costs incurred to ensure the safe handling of the product, and **is liable** for any harm or injury to Varian employees as well as to any third party occurring as a result of exposure to toxic or hazardous materials present in the product.

Do not write below this line

Notification (RA)#: Customer ID#: Equipment #:

FAILURE REPORT

TURBO PUMPS and TURBOCONTROLLERS

<input type="checkbox"/> Does not start <input type="checkbox"/> Does not spin freely <input type="checkbox"/> Does not reach full speed <input type="checkbox"/> Mechanical Contact <input type="checkbox"/> Cooling defective	<input type="checkbox"/> Noise <input type="checkbox"/> Vibrations <input type="checkbox"/> Leak <input type="checkbox"/> Overtemperature	POSITION <input type="checkbox"/> Vertical <input type="checkbox"/> Horizontal <input type="checkbox"/> Upside-down <input type="checkbox"/> Other:	PARAMETERS Power: Rotational Speed: Current: Inlet Pressure: Temp 1: Foreline Pressure: Temp 2: Purge flow:
TURBOCONTROLLER ERROR MESSAGE:			OPERATION TIME:

ION PUMPS/CONTROLLERS

<input type="checkbox"/> Bad feedthrough <input type="checkbox"/> Vacuum leak <input type="checkbox"/> Error code on display	<input type="checkbox"/> Poor vacuum <input type="checkbox"/> High voltage problem <input type="checkbox"/> Other
Customer application:	

VALVES/COMPONENTS

<input type="checkbox"/> Main seal leak <input type="checkbox"/> Solenoid failure <input type="checkbox"/> Damaged sealing area	<input type="checkbox"/> Bellows leak <input type="checkbox"/> Damaged flange <input type="checkbox"/> Other
Customer application:	

LEAK DETECTORS

<input type="checkbox"/> Cannot calibrate <input type="checkbox"/> Vacuum system unstable <input type="checkbox"/> Failed to start	<input type="checkbox"/> No zero/high background <input type="checkbox"/> Cannot reach test mode <input type="checkbox"/> Other
Customer application:	

INSTRUMENTS

<input type="checkbox"/> Gauge tube not working <input type="checkbox"/> Communication failure <input type="checkbox"/> Error code on display	<input type="checkbox"/> Display problem <input type="checkbox"/> Degas not working <input type="checkbox"/> Other
Customer application:	

PRIMARY PUMPS

<input type="checkbox"/> Pump doesn't start <input type="checkbox"/> Doesn't reach vacuum <input type="checkbox"/> Pump seized	<input type="checkbox"/> Noisy pump (describe) <input type="checkbox"/> Over temperature <input type="checkbox"/> Other
Customer application:	

DIFFUSION PUMPS

<input type="checkbox"/> Heater failure <input type="checkbox"/> Doesn't reach vacuum <input type="checkbox"/> Vacuum leak	<input type="checkbox"/> Electrical problem <input type="checkbox"/> Cooling coil damage <input type="checkbox"/> Other
Customer application:	

FAILURE DESCRIPTION

(Please describe in detail the nature of the malfunction to assist us in performing failure analysis):

NOTA: Su richiesta questo documento è disponibile anche in Tedesco, Italiano e Francese.
REMARQUE : Sur demande ce document est également disponible en allemand, italien et français.
HINWEIS: Auf Aufrage ist diese Unterlage auch auf Deutsch, Italienisch und Französisch erhältlich.

Sales and Service Offices

France and Benelux

Varian s.a.

7 Avenue des Tropiques
Z.A. de Courtaboeuf - B.P. 12
Les Ulis cedex (Orsay) 91941
France
Tel: (33) 1 69 86 38 84
Fax: (33) 1 69 86 29 88
From Benelux Tel: (31) 118 67 15 70
From Benelux Fax: (31) 118 67 15 69

Canada

Central coordination through:

Varian Vacuum Technologies

121 Hartwell Avenue
Lexington, MA 02421
USA
Tel: (781) 861 7200
Fax: (781) 860 5437
Toll Free # 1 (800) 882 7426

China

Varian Technologies - Beijing

Rm 1648 Central Tower South Wing
Beijing Junefield Plaza
No. 10 XuanWuMenWai Street
Beijing 100052
P.R. China
Tel: (86) 10 63108550
Fax: (86) 10 63100141
Toll Free: 800 820 6556

Germany and Austria

Varian Deutschland GmbH

Alsfelder Strasse 6
Postfach 11 14 35
64289 Darmstadt
Germany
Tel: (49) 6151 703 353
Fax: (49) 6151 703 302

India

Varian India PVT LTD

101-108, 1st Floor
1010 Competent House
7, Nangal Raya Business Centre
New Delhi 110 046
India
Tel: (91) 11 28521171
Fax: (91) 11 28521173

Italy

Varian Inc.

Vacuum Technologies

Via F.lli Varian 54
10040 Leini, (Torino)
Italy
Tel: (39) 011 997 9 111
Fax: (39) 011 997 9 350

Japan

Varian Vacuum Technologies

Sumitomo Shibaura Building, 8th Floor
4-16-36 Shibaura
Minato-ku, Tokyo 108
Japan
Tel: (81) 3 5232 1253
Fax: (81) 3 5232 1263
Toll Free: 0120 655 040

Korea

Varian Technologies Korea, Ltd

Shinsa 2nd Bldg. 2F
966-5 Daechi-dong
Kangnam-gu, Seoul
Korea 135-280
Tel: (82) 2 3452 2452
Fax: (82) 2 3452 2451
Toll Free: 080 222 2452

Mexico

Varian, S. de R.L. de C.V.

Concepcion Beistegui No 109
Col Del Valle
C.P. 03100
Mexico, D.F.
Tel: (52) 5 523 9465
Fax: (52) 5 523 9472

Taiwan

Varian Technologies Asia Ltd.

14F-6, No.77, Hsin Tai Wu Rd., Sec. 1
Hsi chih, Taipei Hsien
Taiwan, R.O.C.
Tel: (886) 2 2698 9555
Fax: (886) 2 2698 9678
Toll Free: 0800 051342

UK and Ireland

Varian Ltd.

6 Mead Road
Oxford Industrial Park - Yarnton
Oxford OX5 1QU - England
Tel: (44) 1865 291570
Fax: (44) 1865 291571

United States

Varian Vacuum Technologies

121 Hartwell Avenue
Lexington, MA 02421
USA
Tel: (781) 861 7200
Fax: (781) 860 5437

Other Countries

Varian Inc.

Vacuum Technologies

Via F.lli Varian 54
10040 Leini, (Torino)
Italy
Tel: (39) 011 997 9 111
Fax: (39) 011 997 9 350

Customer Support & Service:

North America

Toll-Free: 1 800 882 7426
vtl.technical.support@varianinc.com

Europe

Tel: 00 800 234 234 00
vtt.technical.support@varianinc.com

China

Toll-Free: 800 820 8266
vtc.technical.support@varianinc.com

Japan

Toll-Free: 0120 655 040
vtj.technical.support@varianinc.com

Korea

Toll-Free: 080 222 2452
vtk.technical.support@varianinc.com

Taiwan

Toll-Free: 0 800 051 342
vtw.technical.support@varianinc.com

Worldwide Web Site, Catalog and Order On-line:

www.varianinc.com

Representative in most countries



VARIAN